


RXU-8A

Quick Start Guide for MT



RXU-8A (components)	2
Product description	3
Calibration - Config Files	4
MT acquisition	5
Electric Channel Settings	6
Magnetic Channel Settings	7
Sparse high frequency sampling	8
Saving a MT Configuration File	9
RXU-8A Connections	10
Start the Recording	11
Stopping a recording	12
Importing - Field QC	13
Field QC	14
Processing MT Data	15
Viewing Recording Details	16
Technical Support	17

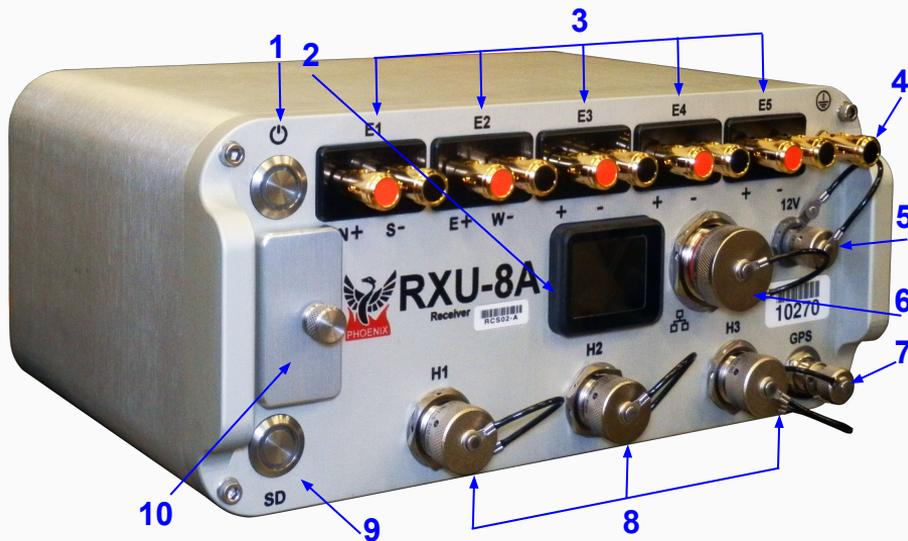

Components

1	Power/Record button and indicator
2	Display
3	E1 (Ex) electrode connectors E2 (Ey) electrode connectors E3 electrode connectors E4 electrode connectors E5 electrode connectors
4	Ground electrode connector
5	12V DC power input
6	LAN connector
7	GPS antenna connector
8	H1 (Hx) magnetic sensor connector H2 (Hy) magnetic sensor connector H3 (Hz) magnetic sensor connector
9	SD card button and indicator
10	SD card slot and cover

RXU-8A



Designed with flexibility in mind, the RXU-8A can be used as a regular MT receiver, where the extra electric channels can be used to acquire a redundant recording on the same site or to acquire an adjacent site.

Excellent choice for controlled source acquisitions that require a large density of electric channels. The RXU-8A can also work for special applications where extra electric inputs might be needed.

This manual is intended for MT operations. The RXU-8A can also be used for CSAMT recordings. For more information on CSAMT consult the [*CSAMT Operation manual*](#) (DAA31).

Calibration - Config Files

Perform the Receiver and Sensors calibrations at start of each installation layout, to ensure the instruments are measuring correctly. Calibration verify the working state of the equipment and helps to improve the quality of the records and the reliability of the measurements.





Open **EMpower** and select the **Prepare** module

1. Sensor

- 1.1. Click the Sensor button and choose the magnetic channels that will be used
- 1.2. Select the **Sensor Type**
- 1.3. Type the **Serial number**, (*not needed for MTC-155/MTC-185 sensors*)
- 1.4. Or **Load** it from a previous config file
- 1.5. **Save** the configuration file (config.json) in the SD card (*see page 7*)

2. Receiver

- 2.1. Select the **Receiver Type** and click the **Receiver** button
- 2.2. **Save** the configuration file (config.json) in the root folder of the SD card (*see page 7*)

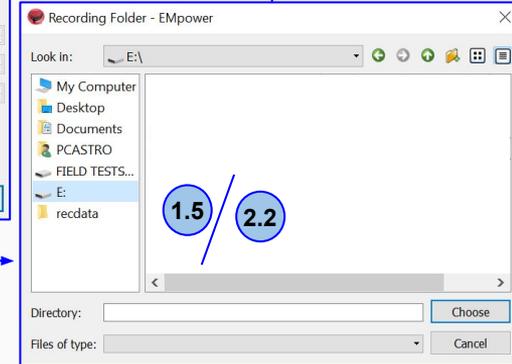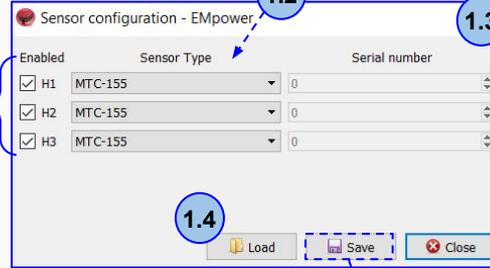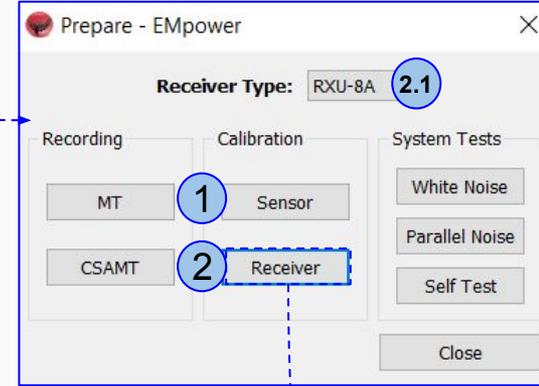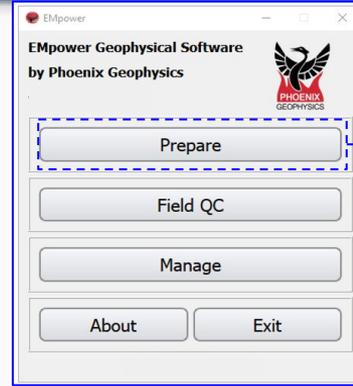

For more details consult [DAA22-Guide For MT Field Operations](#)

Creating a Configuration file - MT acquisition

1. Click **Prepare** and select the **Receiver Type** as **RXU-8A** and click the **MT** button

2. Select the **Schedule**

1.1. **Manual** or **Automatic Start**

1.2. Or for a specific schedule use, **Single Shot**, **Daily** or **Weekly**. To set scheduled times and dates, click **Add Schedule**

3. **Ethernet port** (consult the [Remote Networking](#) manuals)

4. Define the **Channel Settings** (See pages 6, 7)

○ Define the **Receiver Settings**

○ **Sampling Mode**

- *Continuous Sampling* (Applicable to research studies)

- *Sparse high frequency sampling* (See [Frequency sampling page](#))

○ **Sampling Rate**

○ **Power Recovery** (consult the [Power Recovery](#) manuals)

5. **Configuration Layout**

1

2

2.1

2.2

3

4

5

6

! This section is used for inputting the parameters and instrument details that will be used for the recording

To use the magnetic sensor data from a different recording or use a remote reference, all recordings **must** have a matching Sampling Mode and Sampling Rates. Otherwise, EMpower will not allow to process data using borrowed channels or remote reference

Electric Channel Settings

1. Select the **Electric** channel

2. Enable or **Disable** channel(s)

- Disable channels that you do not plan to use during the recording. This will save space on the SD card.

3. Select the desired **Gain** and **Low Pass Filter**


- For most applications, Normal Gain and 10 kHz LPF are best

4. Type **distances to the electrodes** of this channel if known

- If not, they will need to be corrected later before data processing



Some settings can be configured by using the right-click menu

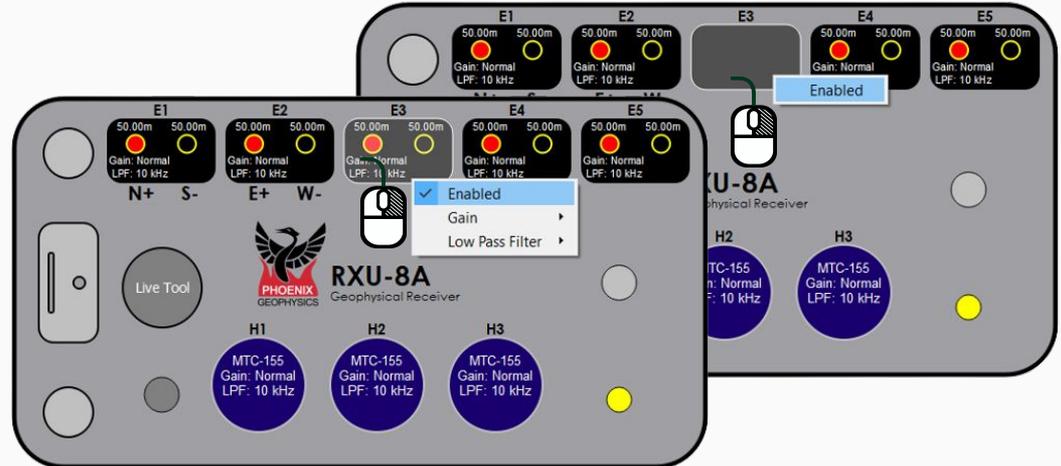

Magnetic Channel Settings

1. Select a **Magnetic** channel

2. **Enable or Disable** channel(s)

- Disable channels that you do not plan to use during the recording. This will save space on the SD card.

3. Select the correct **Sensor Type**


- If the sensor type is incorrect in the configuration file, the receiver will display a warning message. However, the recording will not be interrupted

4. Select the desired **Gain** and **LPF**


- For most broadband applications with MTC-100 series sensors, Normal Gain and 10 kHz LPF are best

5. Type the **Serial Number** of the sensor if required

- There is no need to type serial number for sensors MTC-155/MTC-185, since it will be automatically detected by the receiver.
- For older sensors, type the serial number of each sensor. If you don't know this information in advance, keep field notes to add this information later, after the recording is imported into EPower

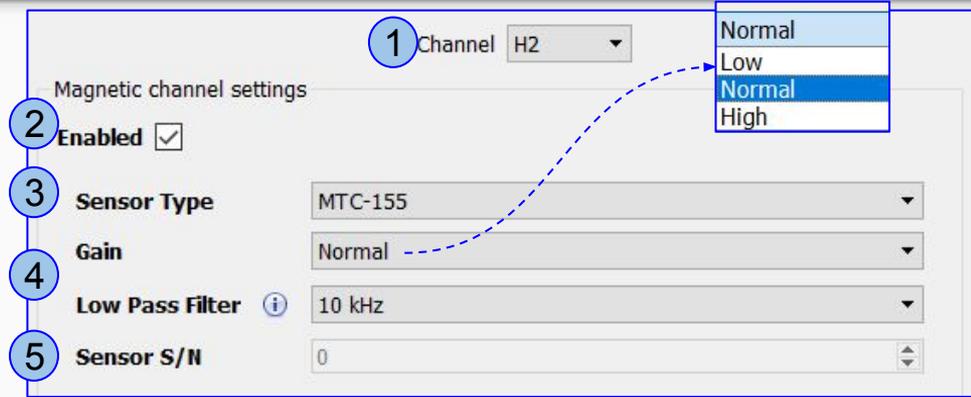

2 Some settings can be configured by using the right-click menu

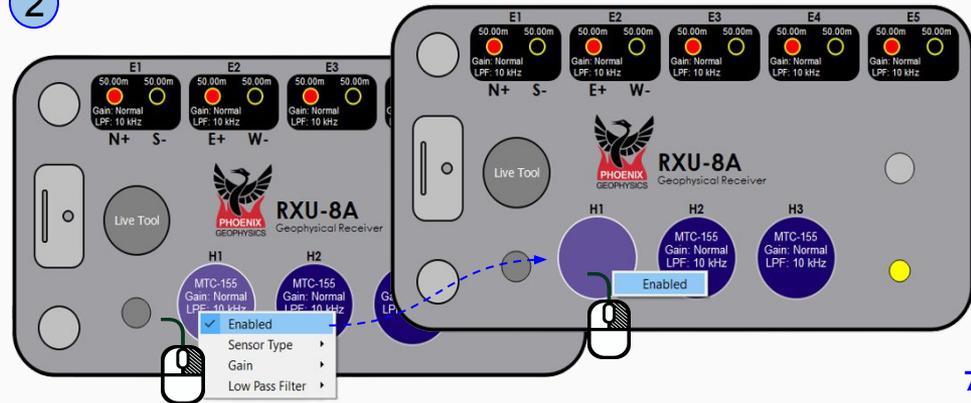

Sparse high frequency sampling- MT acquisition


Sparse high frequency sampling combined with varying **Sampling Rates** is used for common industrial applications such as oil and gas exploration, geothermal exploration, reservoir monitoring, and geotechnical studies.

1. Select **Sparse high frequency sampling** and choose the **Sampling Rate**
2. Enable the **View graphic** to visualize on the left side how the Sampling Rate options work




2.1. 24 ksp/s High, use this option for environments with varying or moderate noise levels (*overnight recordings*)

2.2. 24 ksp/s Low, use this option for areas where noise levels are consistently low (*overnight recordings*)

2.3. For remote sites requiring extensive recordings, use the **24 ksp/s Longterm** option to enable weekly or monthly log recordings while minimizing SD card space usage
**Recommended for working with network remote access.*

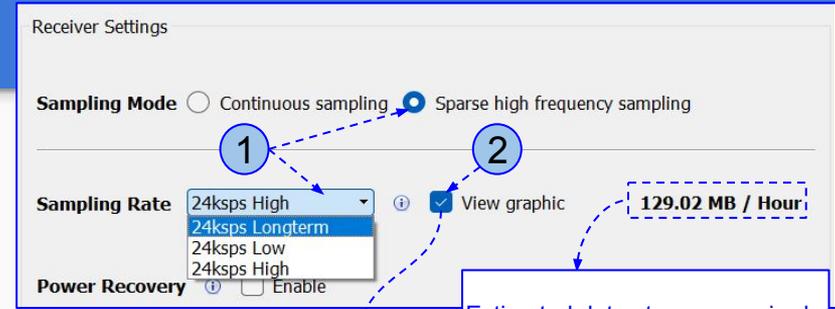

Estimated data storage required per hour based on sampling rate

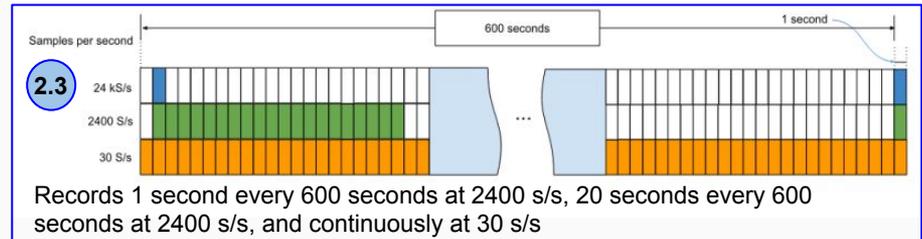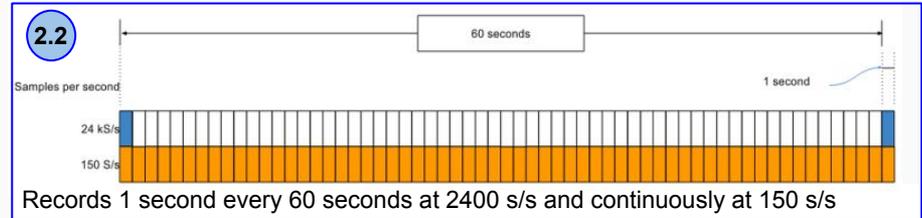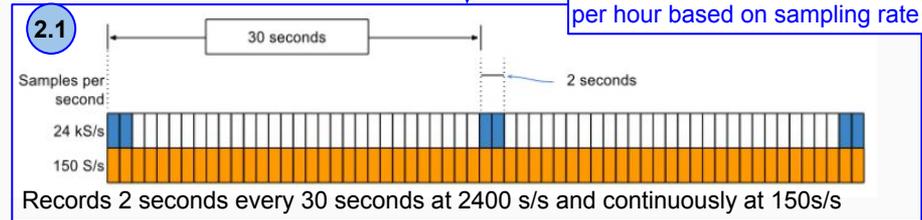

Saving a MT Configuration File

1. Insert the SD Card

- The computer must be equipped with an SD card slot or use a USB card reader




2. Click the **File** menu

- Save or **Ctrl+S**
- Select the SD card
- **EMpower** will automatically create the file "**config.json**"

3. Save the configuration file (*config.json*) in the root folder of the **SD card**

4. Open the file explorer

- Right click **SD card** drive
- **Select Eject option**
- **Pull out the SD Card**

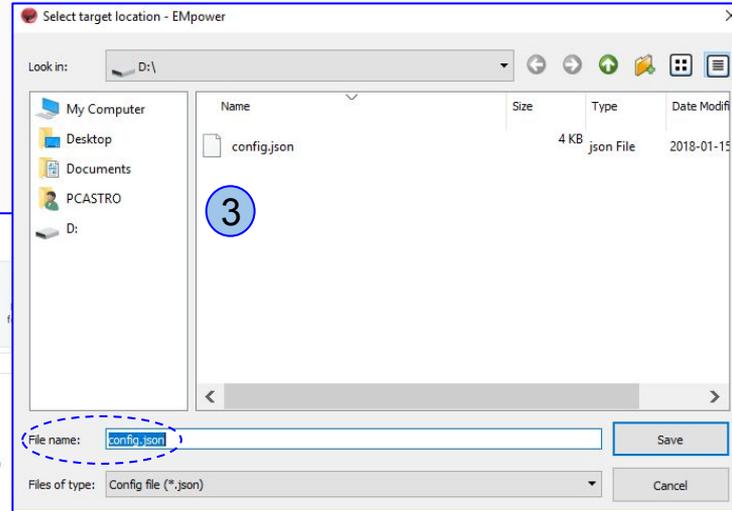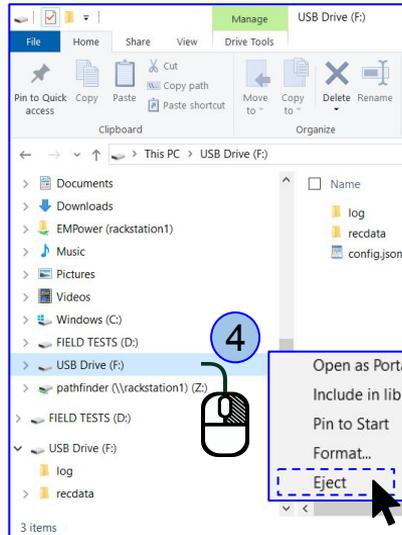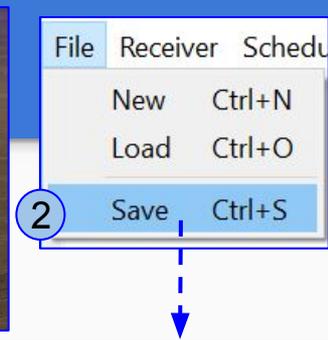



RXU-8A

Connection - Single site MT

Start by connecting:

1. Ground electrode
2. Electrodes to channel **E1**(Ex) (N+, S-) and channel **E2**(Ey) (E+, W-)
 - Channels E3, E4, E5 are normally not required in a conventional Single site MT survey
3. Magnetic sensors to channels **H1**(Hx), **H2**(Hy) and **H3**(Hz)
4. GPS antenna
5. 12V DC Power Source
6. Network connector

i In the field, it is often most efficient to connect the components to the receiver following the order on the right

Start the Recording

Before starting a recording, execute the calibration of the receiver and sensors to verify the operating status of the equipment and ensure the quality of the recordings and the reliability of the measurements.

*For more details consult [DAA22- Guide For MT Field Operations](#)

1. Insert the **SD card** and close the cap
2. To turn on the receiver, press the **Power** button briefly, wait until both **LEDs** are solid blue
 - 2.1. LED pattern for **Automatic Start** recording
3. If the schedule type was configured as **Manual**, press the **Power** button briefly and release to start recording



*For any problems with the SD Card, check the [DAA24 System Troubleshooting manual](#)

i The receiver auto-detects serial and model for magnetic sensors of the new generation (MTC-155/185). The information about the sensor is updated on the receiver screen only at power on and right after each recording starts.

- 2 Briefly press and release the power button



- 2.1 **Automatic Start**
The recording starts automatically according to the schedule



- 3 Briefly press and release the power button



Indicators

  *Slow, equal pulses*
 *Solid color / Off*

Stopping a recording

1. Press the **Power** button briefly and release to stop recording
 - Wait until both **LEDs** are steady blue
2. Turn off the receiver by pressing the **Power** button for a few seconds, until the **LEDs** will flash red
 - Wait until both **LEDs** turn off
3. Eject the **SD card**
 - Press the **SD card** and release, pull the **SD card**

- 1 Press the **Power** button briefly and release



- 2 Keep pressing the power button 3 sec and release



- 3








Indicators

■■■■■■■■ *Rapid, equal pulses*
■■■■■■■■ *Solid color / Off*

Importing - Field QC

- 1. Click the **Field QC** button
- 2. Select **View data**
- 3. Select the **SD card**
 - o The recording creates two folders, **log** and **recdata**
- 4. Open the **recdata** folder
 - o Select the recording file
 - o Click **Choose**

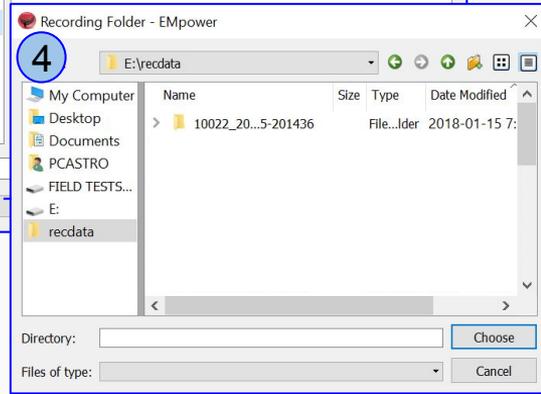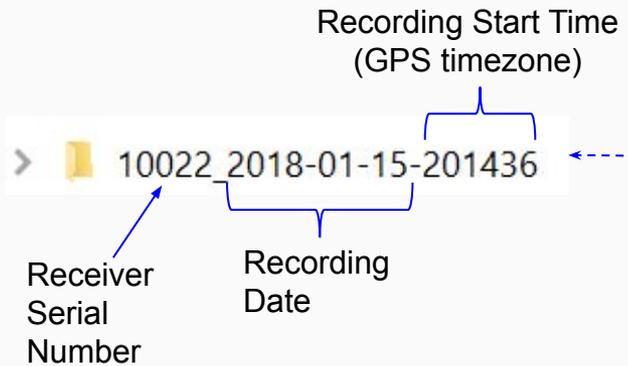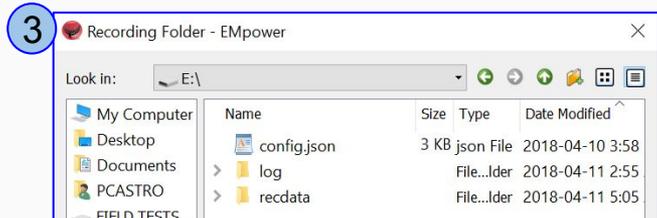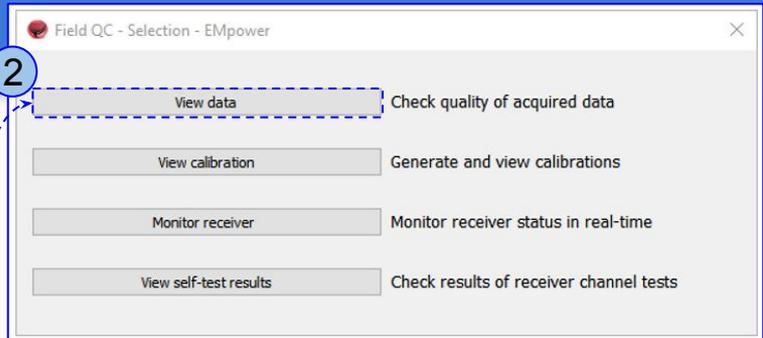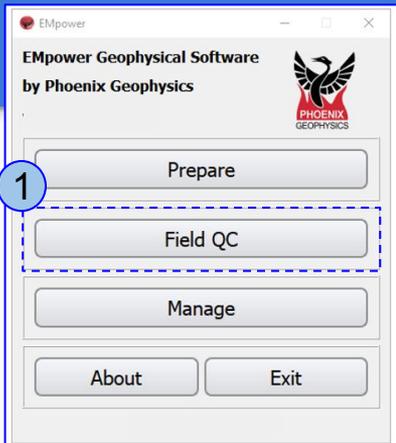

1. Review the **Recording Information**
2. Review the Electrode **Resistance** values and make the necessary corrections
 - Electrode **Distance (m) to GND**
 - **Polarity**
 - **E Azimuth**
 - **External Filter**
3. Ensure that the magnetic sensors were detected and make the necessary corrections
 - **Serial #**
 - **Polarity**
 - **H1-H3 Azimuth**
 - **H4-H6 Azimuth**
4. View Recording Details (see page 15)
5. After reviewing the information, **Process** the data



The warning icon indicates that something might be wrong with the recording, review the recording information and make necessary changes if needed. Hover mouse pointer over the warning icon for more information.

Recording Information

Recording ID: 10125_2017-12-03-203322

Start time: Dec 03 2017 12:33:24 (Local) Eastern Standard Time (GPS -08:00)

Duration: 21h 32m 56s

Survey name: Don Campbell

Station name: S7_1_5C

Operator(s): CF MU and GB

Company name:

Layout Geometry: Orthogonal

Declination: 13.00°

Notes:

Electric Channels

Channel	Distance (m) to GND		Polarity	Resistance (Ω)		Gain	LPF [Hz]	DC [V]
	(+) N / E	(-) S / W		(+) N / E	(-) S / W			
E1	50.00	50.00	<input type="checkbox"/> Inverted	235.522	305.681	4 x 4 = x16	10000	-0.011
E2	50.00	50.00	<input type="checkbox"/> Inverted	231.074	305.313	4 x 4 = x16	10000	-0.014

E Azimuth: 40.00 ° External Filter: None

Magnetic Channels

Channel	Sensor	Detected	Serial #	Polarity	Gain	LPF [Hz]	DC [V]
H1	MTC-80H	Not Present		<input type="checkbox"/> Inverted	x4	10000	0.074
H2	MTC-155	MTC-155	53918	<input type="checkbox"/> Inverted	x4	10000	0.032
H3	MTC-155	MTC-155	53195	<input type="checkbox"/> Inverted	x4	10000	-0.078

H1-H3 Azimuth: 40.00 °

View Recording Details

This section can also be used to input additional field information if desired

Processing MT Data

6. Select the local **Reference type** for the channels
7. Select the channels **Manually** button to choose specific channels, this can be done for both magnetic and electric channels
8. Define the segment of time series to be processed, select the **Start** and **End** date/time, or use the arrows to define the time period
9. Select the **electric power grid filter** that corresponds to the frequency carried by the power lines in the survey area (*50Hz, 60Hz, or None*)
10. Click the **Process** button
11. A live display of the resistivity curve will appear after a few seconds

The screenshots illustrate the following steps in the EMpower software:

- Step 6:** Selecting the local **Reference type** (Magnetic) for the channels.
- Step 7:** Selecting the **Manually** button to choose specific channels for both magnetic and electric channels.
- Step 8:** Defining the segment of time series to be processed by selecting the **Start** and **End** date/time.
- Step 9:** Selecting the **electric power grid filter** (60 Hz) that corresponds to the frequency carried by the power lines in the survey area.
- Step 10:** Clicking the **Process** button.
- Step 11:** A live display of the resistivity curve will appear after a few seconds.

Viewing Recording Details

Review that the following levels are within valid limits for quality control:

- 1. Battery Voltage
- 2. Internal Temperature
- 3. Number of Satellites
- 4. Saturated Frames

○ If saturation is not close to ~0%, review the channel configuration (see pages 4 - 6), the channel gain might be too high and/or there is artificial noise on your site

5. Time Series Level

The screenshot shows the EMpower recording details interface. The main window displays recording information for recording ID 102_2018-10-04-193809. Five callouts are present:

- 1. Battery Voltage:** A line graph showing voltage (V) over time, starting at approximately 12.8V and decreasing to about 12.4V.
- 2. Internal Temperature:** A line graph showing temperature (°C) over time, fluctuating between approximately 17.4°C and 20.4°C.
- 3. Number of Satellites:** A bar chart showing the number of satellites over time, with values ranging from approximately 6 to 14.
- 4. Saturated Frames - E1:** A bar chart showing the number of saturated frames over time, with values ranging from 0 to 3.
- 5. Time Series Level - E1:** A scatter plot showing signal level (V) over time, with a legend for Maximum (red), Average (green), and Minimum (blue).

The main interface also includes a table for Channels Details:

Tag	Board S/N	Model	Firmware	Sat	Signal Ranges	
1	E1	201070	BCM01-I	1001c	~0 % - View	View Levels
2	E2	201071	BCM01-I	1001c	0-99 % - View	View Levels
3	H1			0 %	View Levels	
4	H2			0 %	View Levels	



Please check out the [FAQs](#)

<https://phoenixgeophysics.freshdesk.com/>

Or email us at: support@phoenix-geophysics.com